

Advanced Medical Design CO., LTD. 4F~5F, No29, Wuquan 5th Rd., Wuqu Dist ., New Taipei city, 248 Taiwan TEL: 886-2-22902627 FAX: 886-2-22988501

Instruction for Use

Product: Insufflation Filter with Tubing Set

The Following information should be read before using this device.

Intended Use:

To be used in conjunction with MIS procedure kit for intra-abdominal Laparoscopic surgery and procedure.

Note: Single use only, Sterile (Unless package is damaged or opened). All contents are ETO sterilized.

Instruction for Use:

- 1. Tear off cover to access sterile contents.
- 2. Place contents on sterile field.
- 3. Give the connection fitting closest to filter to the nurse for connection to output insufflation gas port.
- 4. For barbed output, simply cut off fitting and insert over barbed fitting.
- Connect the opposite Luer connector in sterile field to Veress Needle or gas port of Surgical Trocar Cannula. 5.
- 6. Proceed with insufflation.


Cautions/Warnings:

This device was designed, tested and manufactured for single patient use only. Reuse or reprocessing of this device may lead to its failure and subsequent patient injury. Reprocessing and/or re-sterilization of this device may create the risk of contamination and patient infection. Do not reuse, reprocess or re-sterilize this device.

Contents sterile unless enclosed package has been opened or damaged. Store at 15°C~25°C.

Dispose used product following local state or federal guidelines.

Federal (U.S.A) law restricts this device to sale, distribution, and use by, or on the order of a physician.

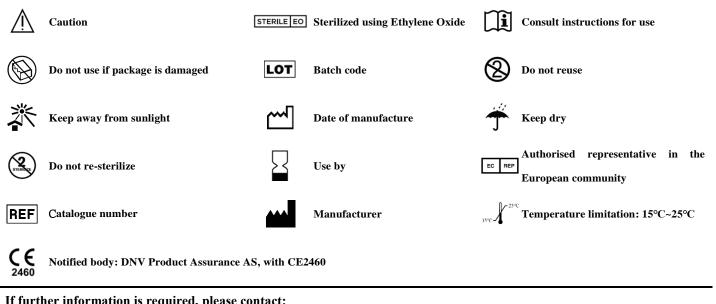

EC REP

If further information is required, please contact:

Advanced Medical Design Co., Ltd. 4F~5F, No29, Wuquan 5th Rd., Wugu Dist., New Taipei City, 24888 Taiwan R.O.C. TEL: 886-2-22902627 FAX: 886-2-22988501 Email: sales@amdintl.com.tw

- **OBELIS S.A** Bd. Général Wahis, 53, 1030 Brussels, Belgium TEL: +3227325954 FAX: +3227326003
- E-mail: mail@obelis.net